

HEIGHT CALIBRATION OF SCANNING PROBE MICROSCOPE ACTUATORS

Osamah M. El Rifai et al.

MIT-135PUS

1/8

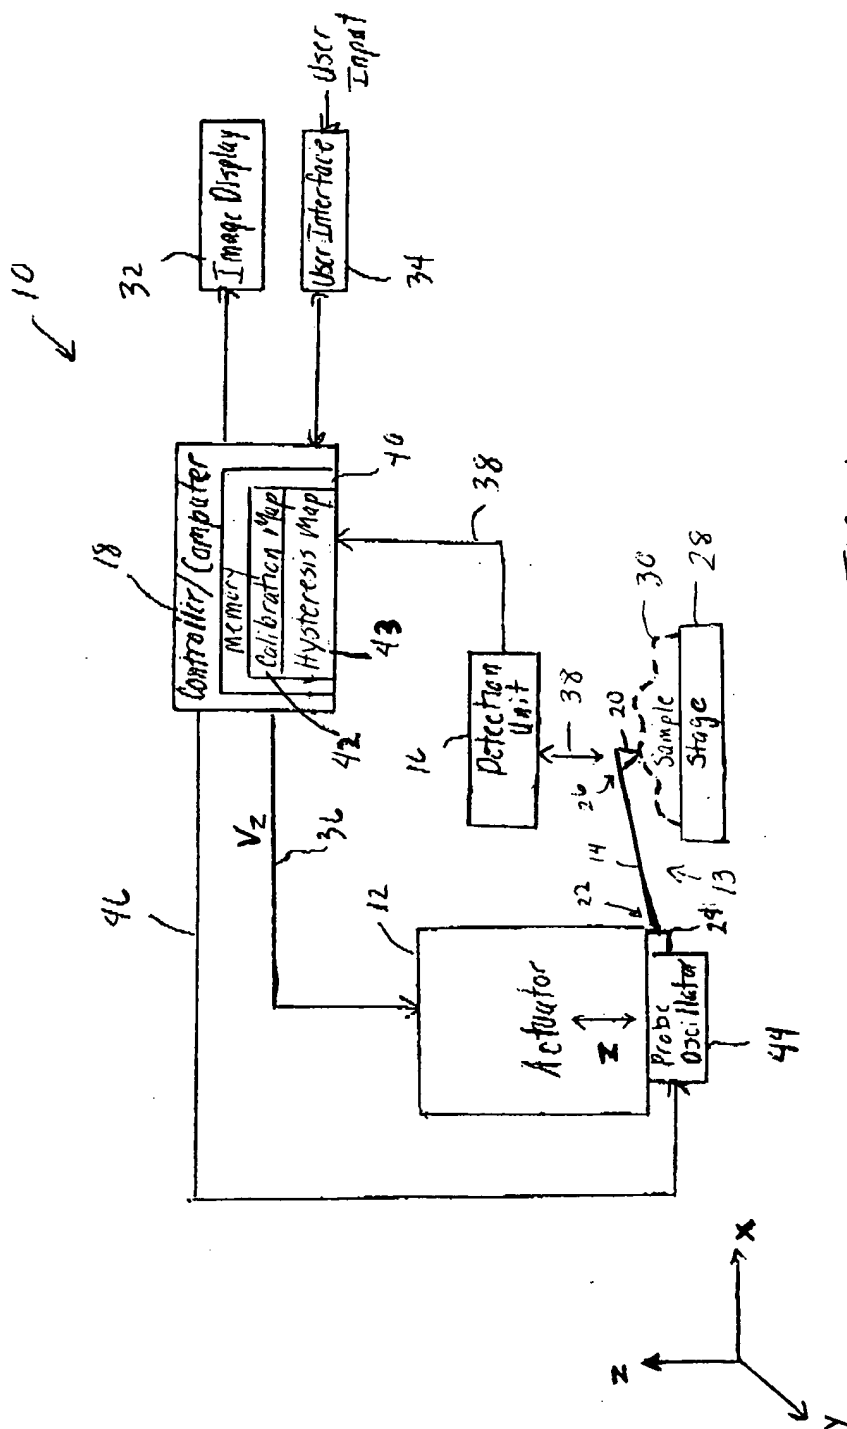


FIG. 1

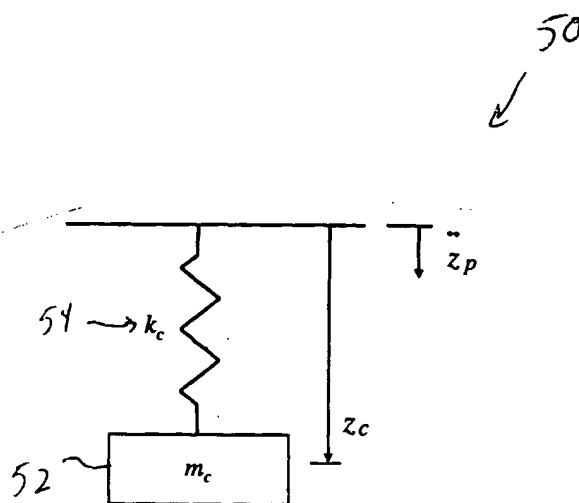


FIG. 2

HEIGHT CALIBRATION OF SCANNING PROBE MICROSCOPE ACTUATORS

Osamah M. El Rifai et al.

MIT-135PUS

3/8

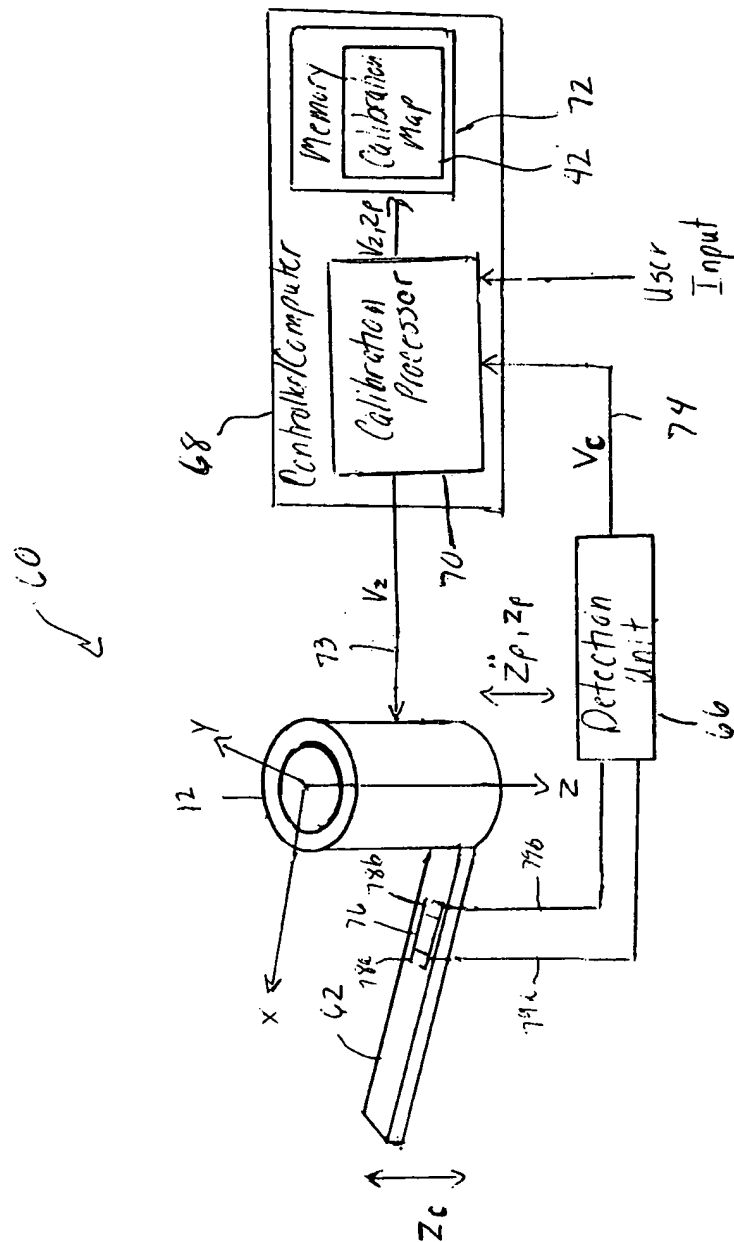


FIG. 3

4/8

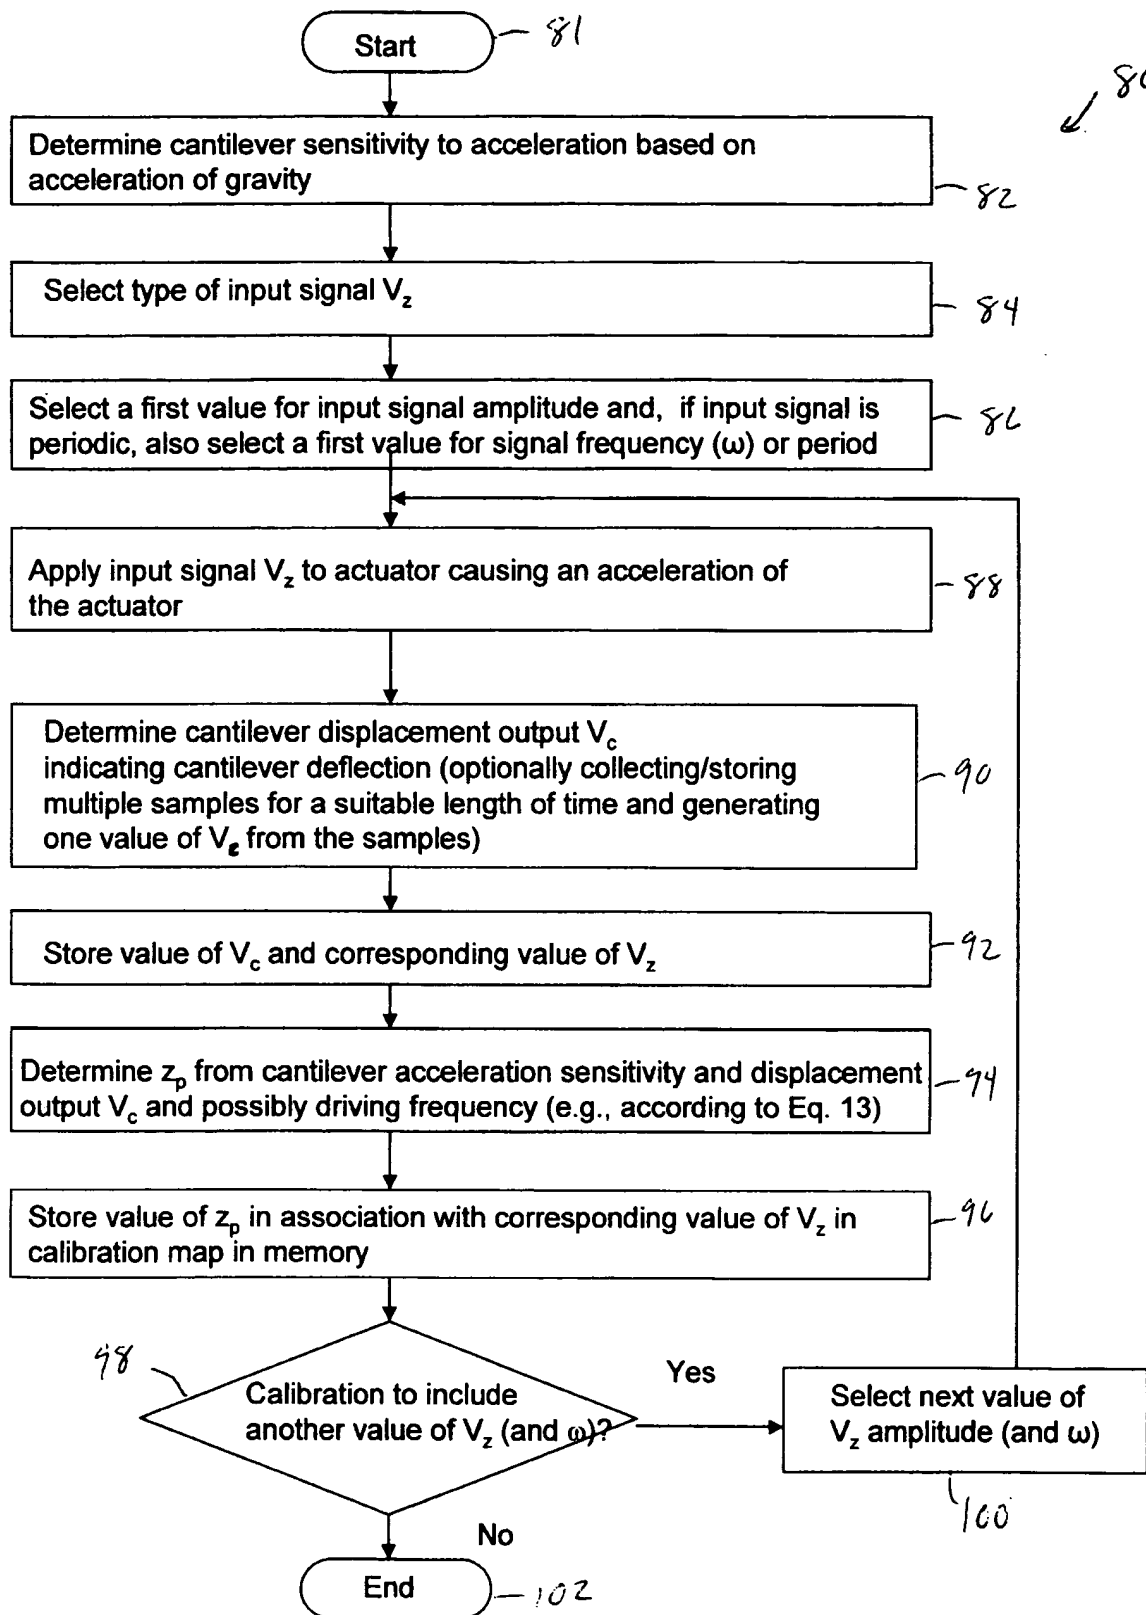


FIG. 4

HEIGHT CALIBRATION OF SCANNING PROBE MICROSCOPE ACTUATORS

Osamah M. El Rifai et al.

MIT-135PUS

5/8

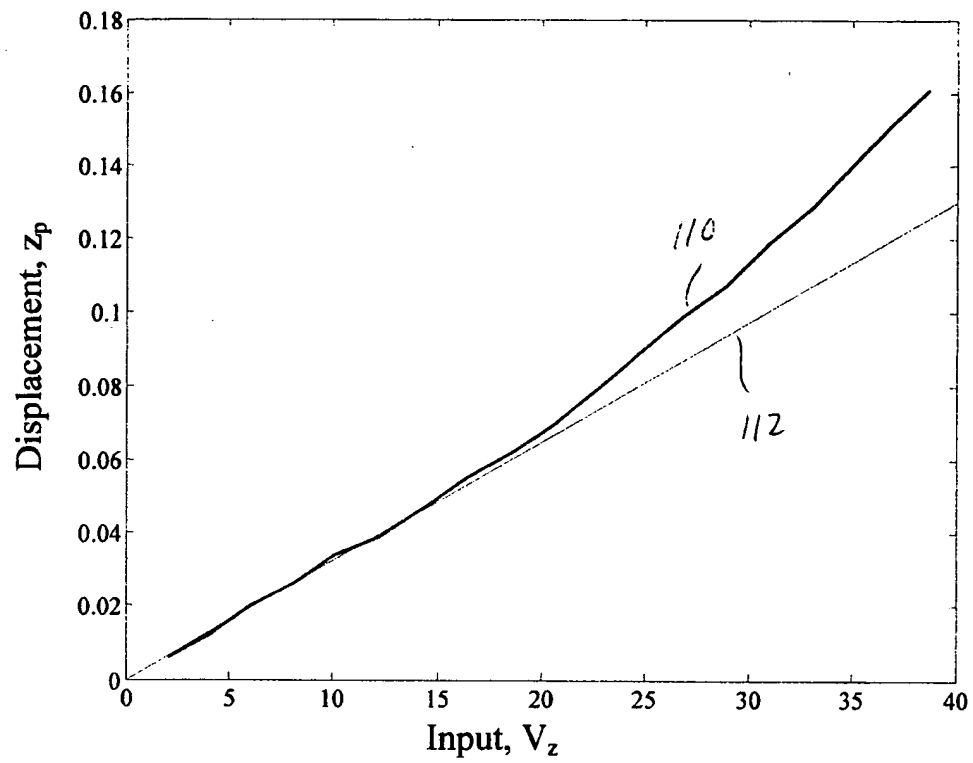


FIG. 5

HEIGHT CALIBRATION OF SCANNING PROBE MICROSCOPE ACTUATORS

Osamah M. El Rifai et al.

MIT-135PUS

6/8

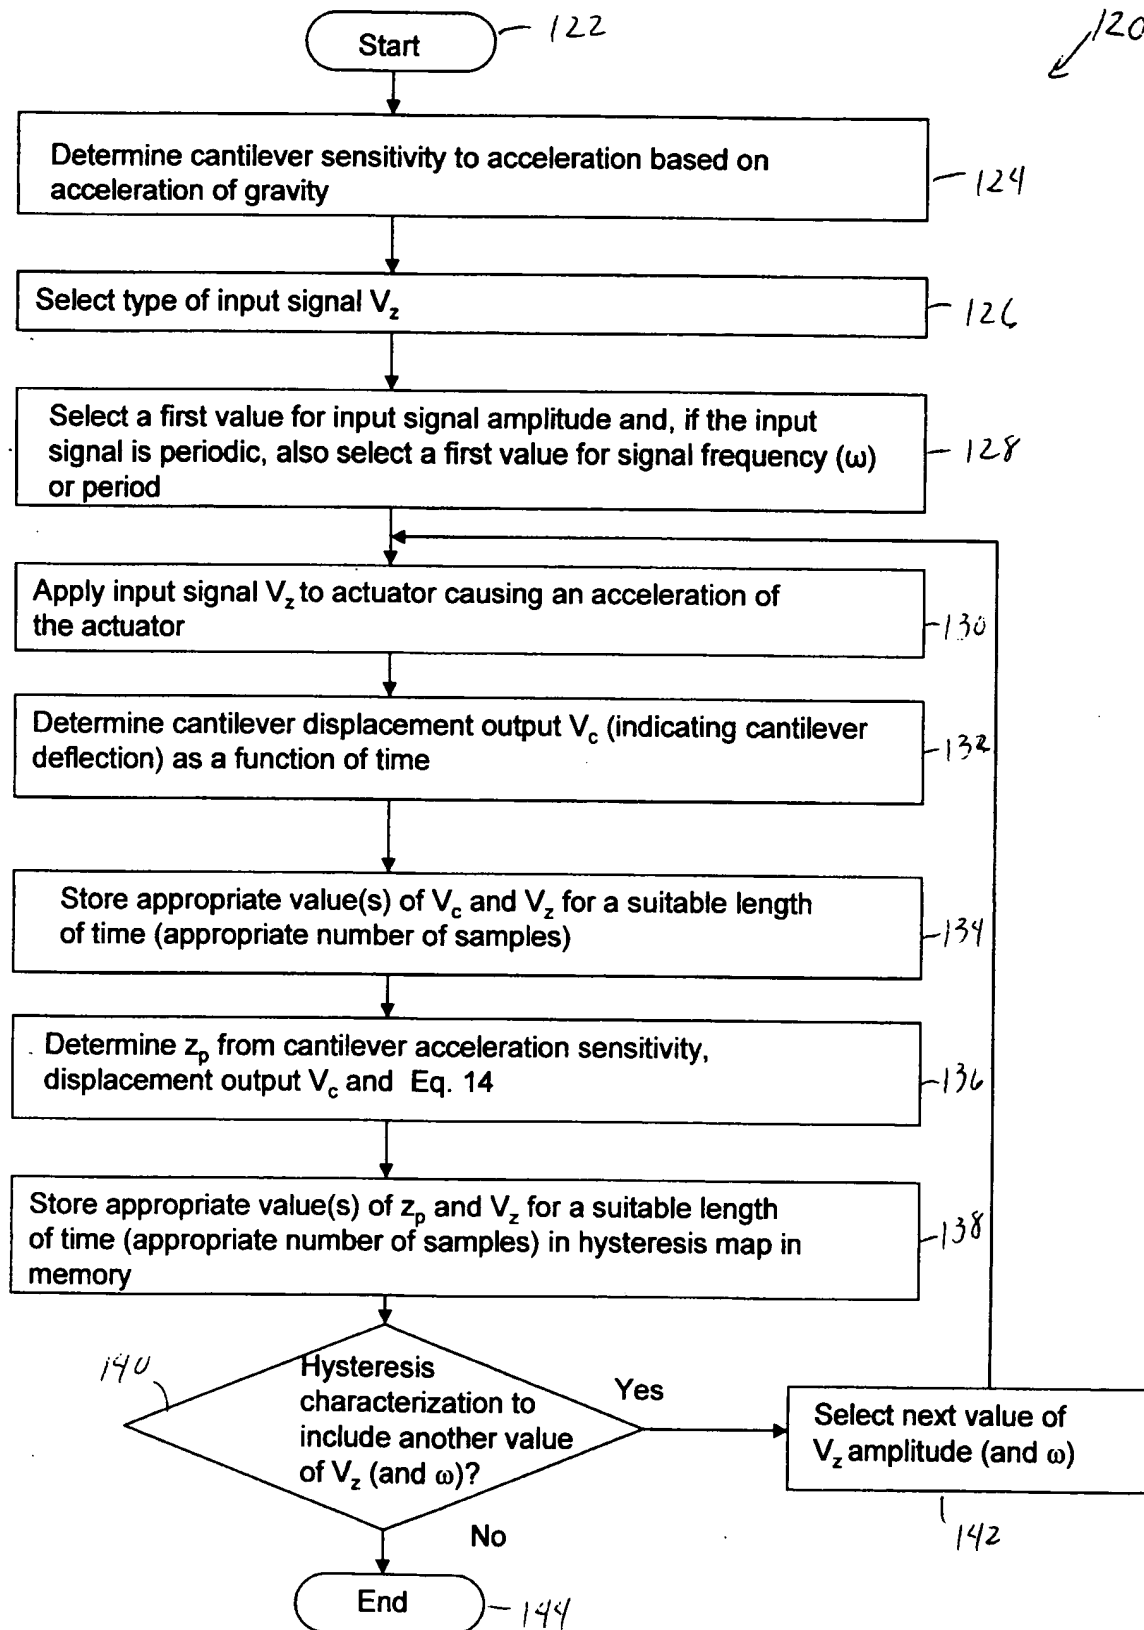


FIG 6

HEIGHT CALIBRATION OF SCANNING PROBE MICROSCOPE ACTUATORS

Osamah M. El Rifai et al.

MIT-135PUS

7/8

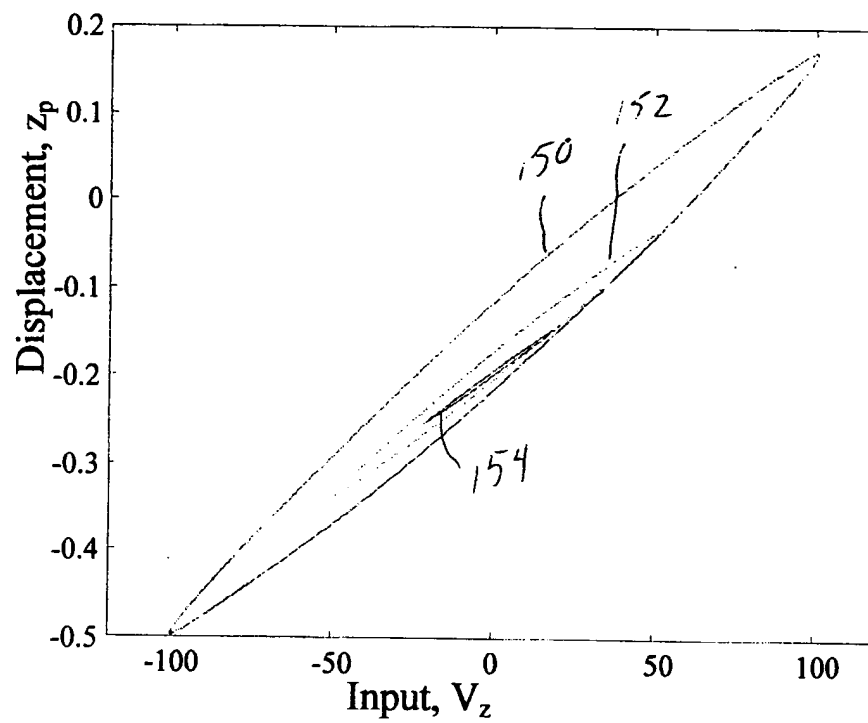


FIG. 7

BEST AVAILABLE COPY

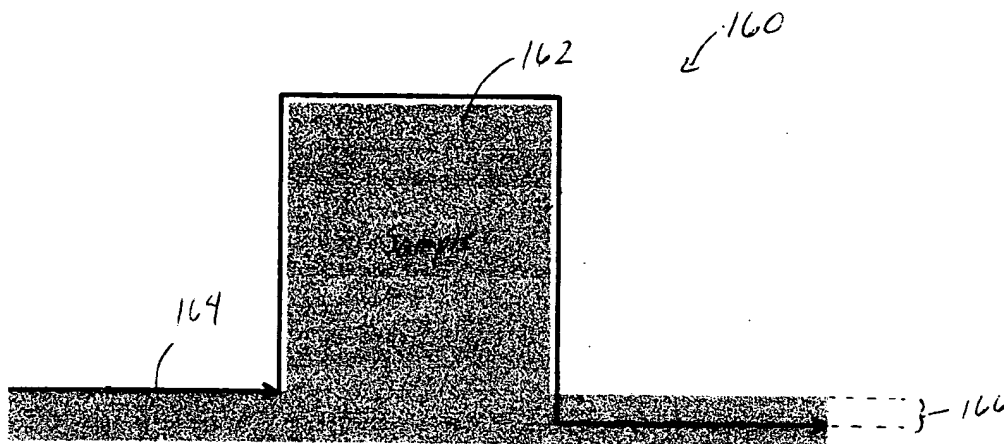


FIG. 8

BEST AVAILABLE COPY